




Riata High Voltage Shock Delivery

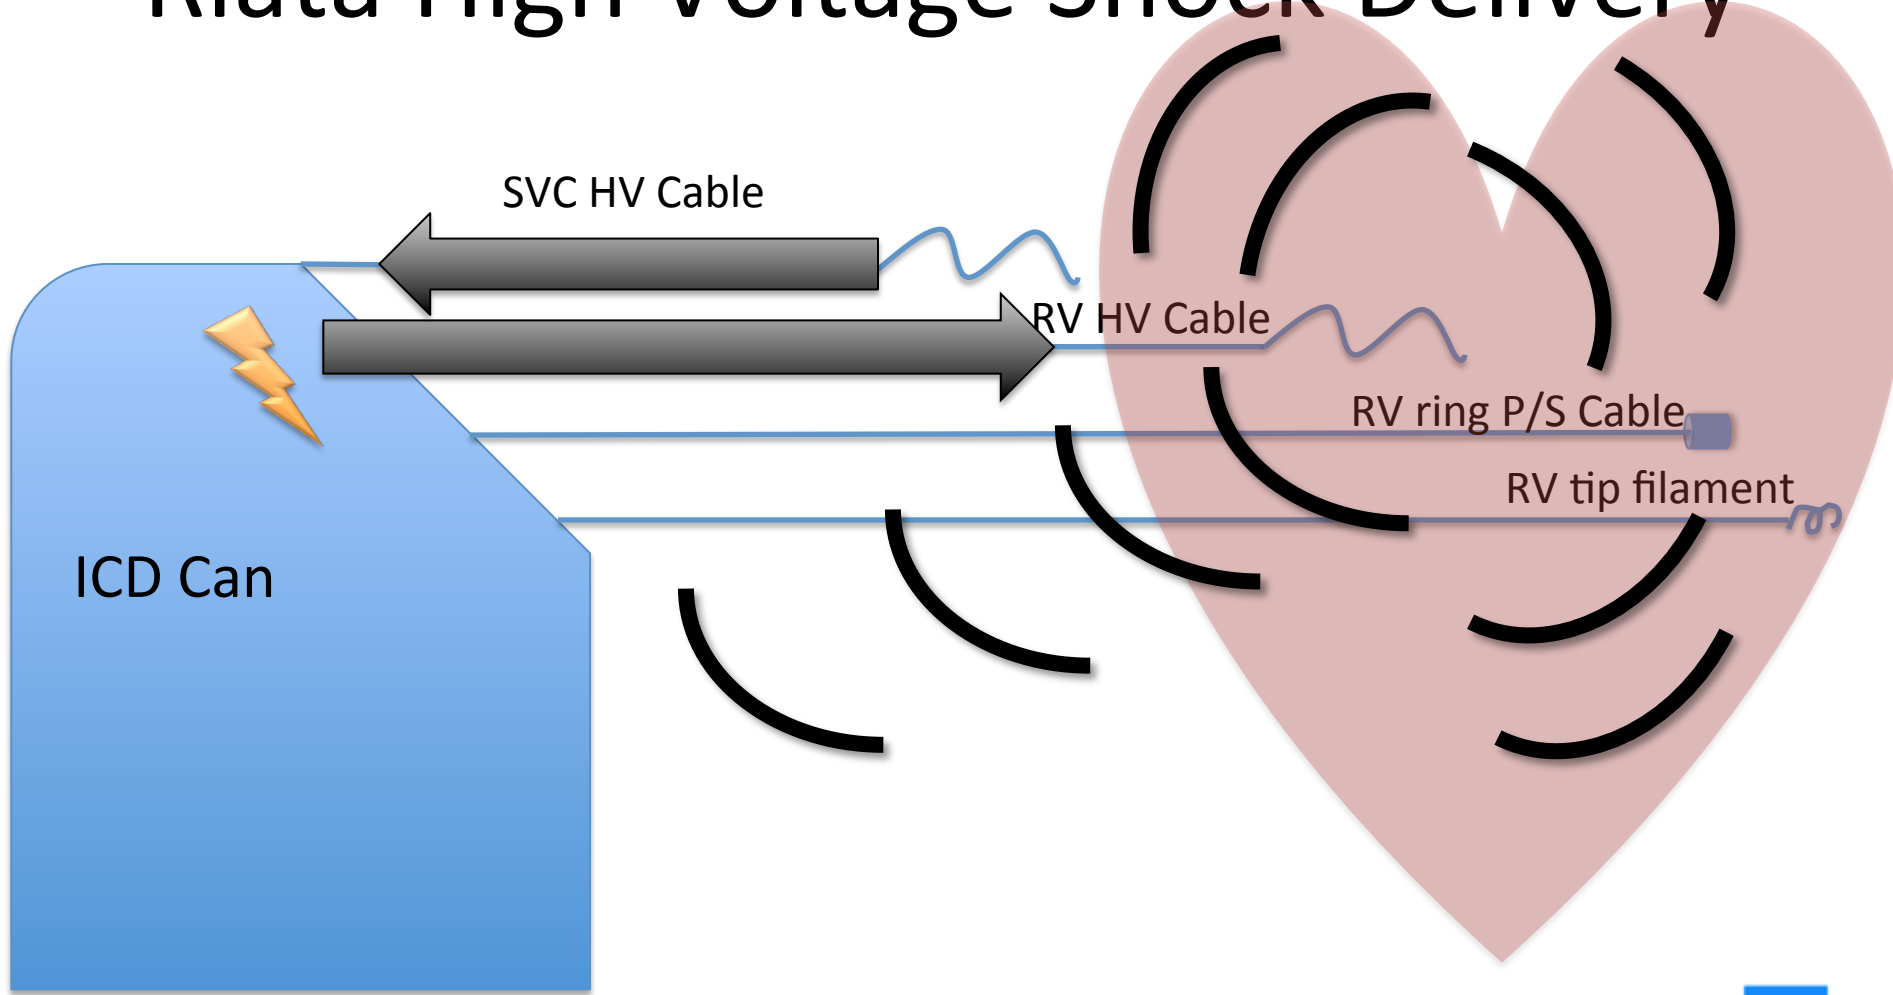

Riata HV Insulation Shorts

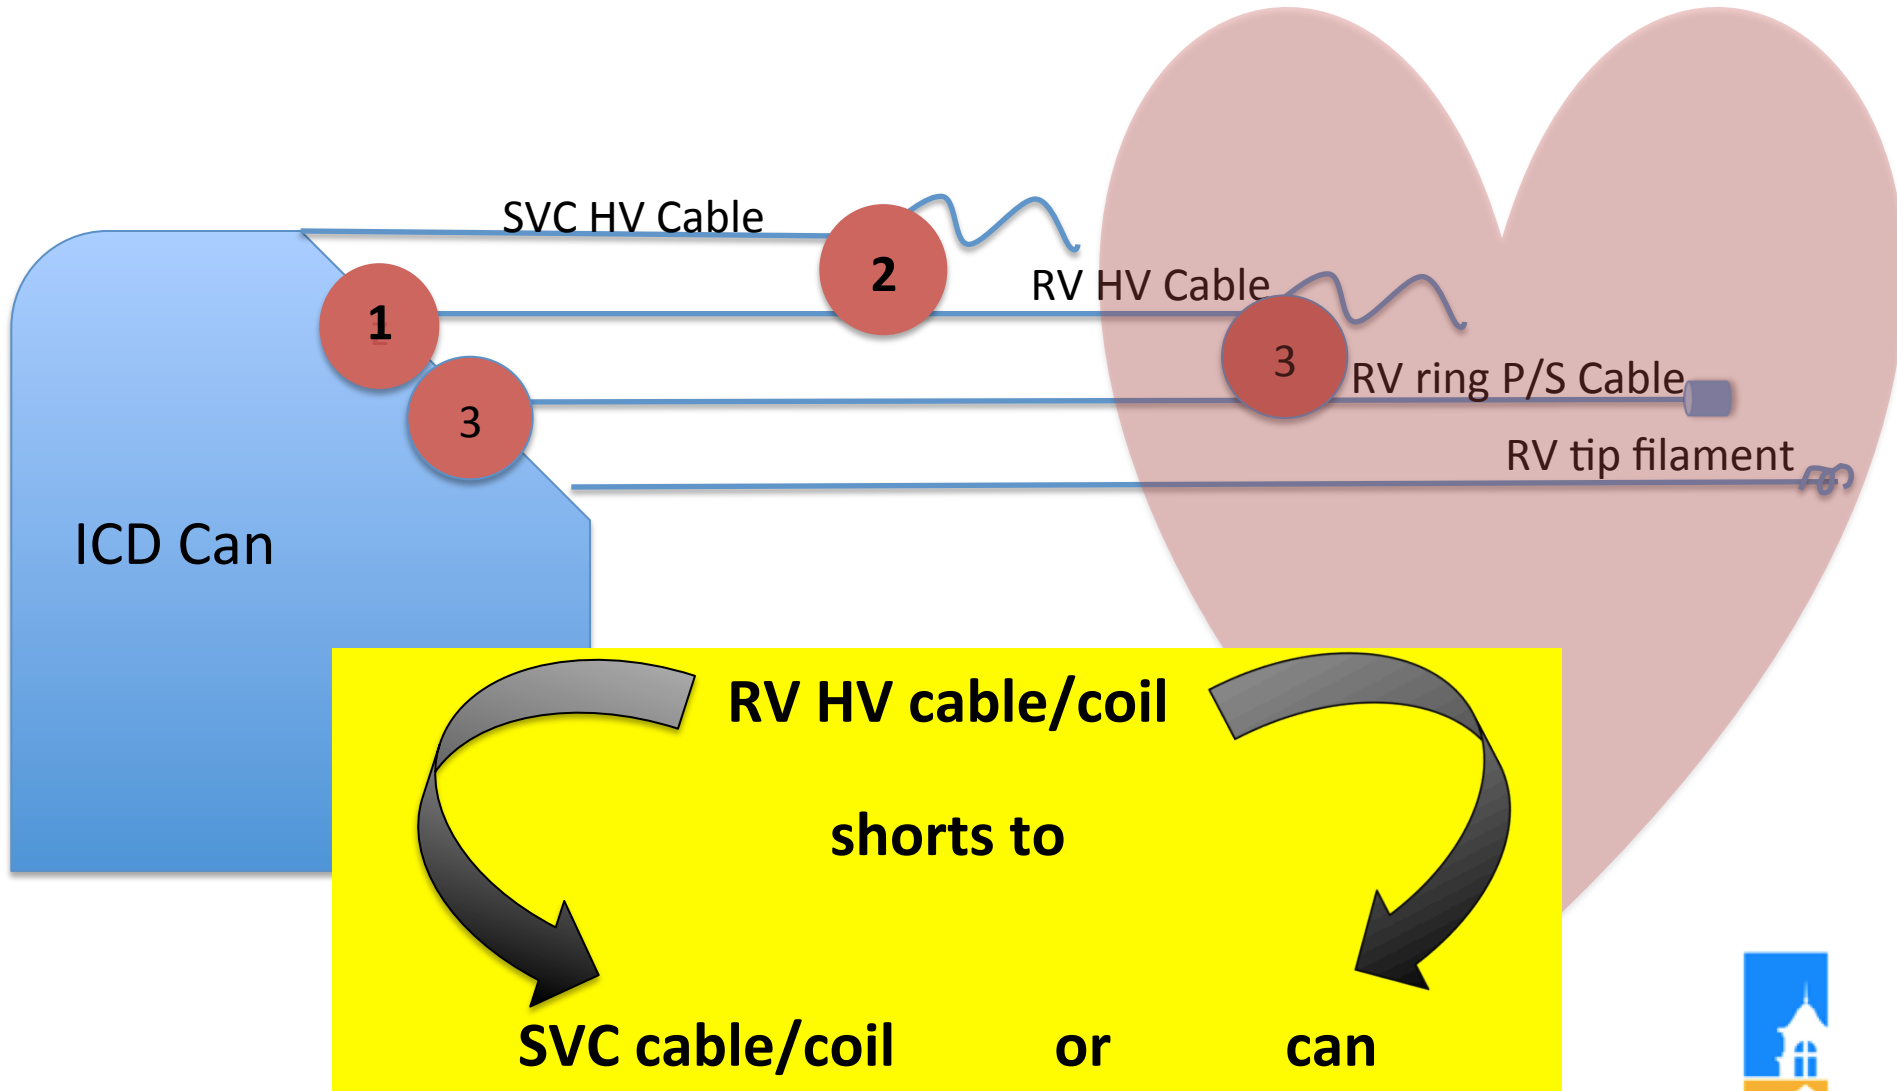

Riata HV Insulation Shorts

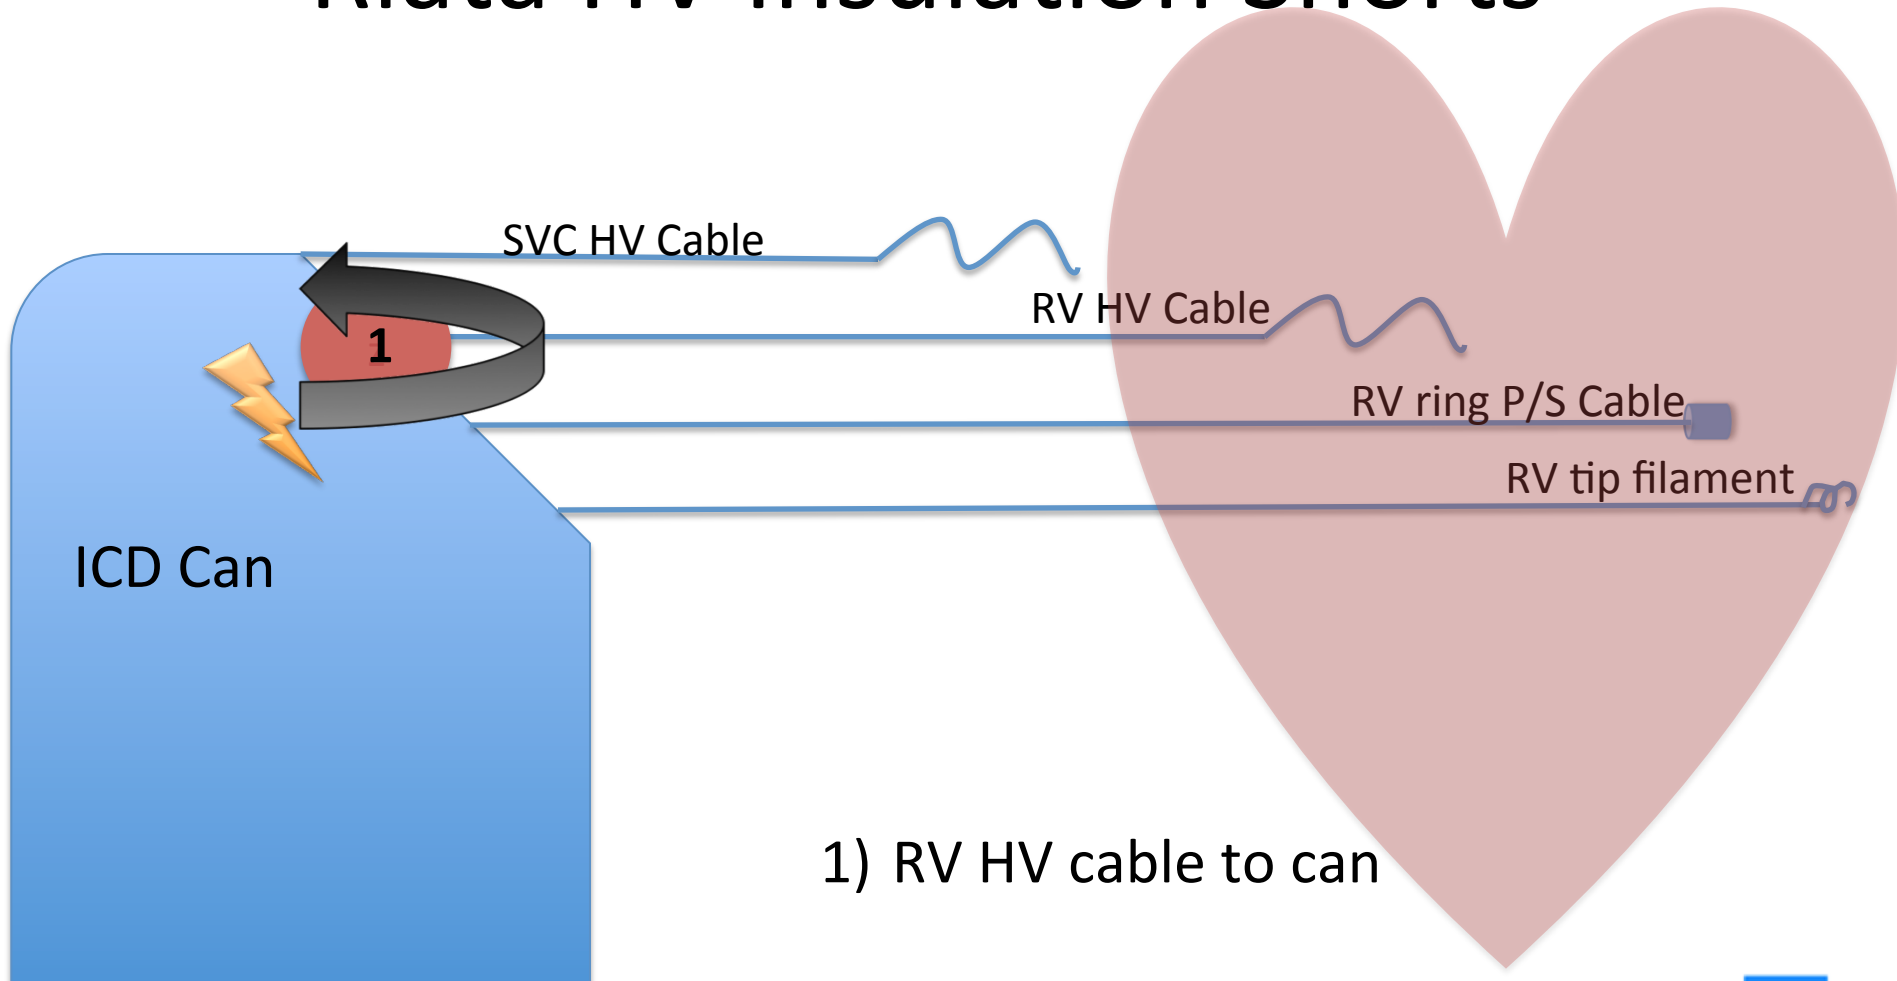


1) RV HV cable to can

Programming the can out of the system may mitigate (if dual coil lead)




Riata HV Insulation Shorts

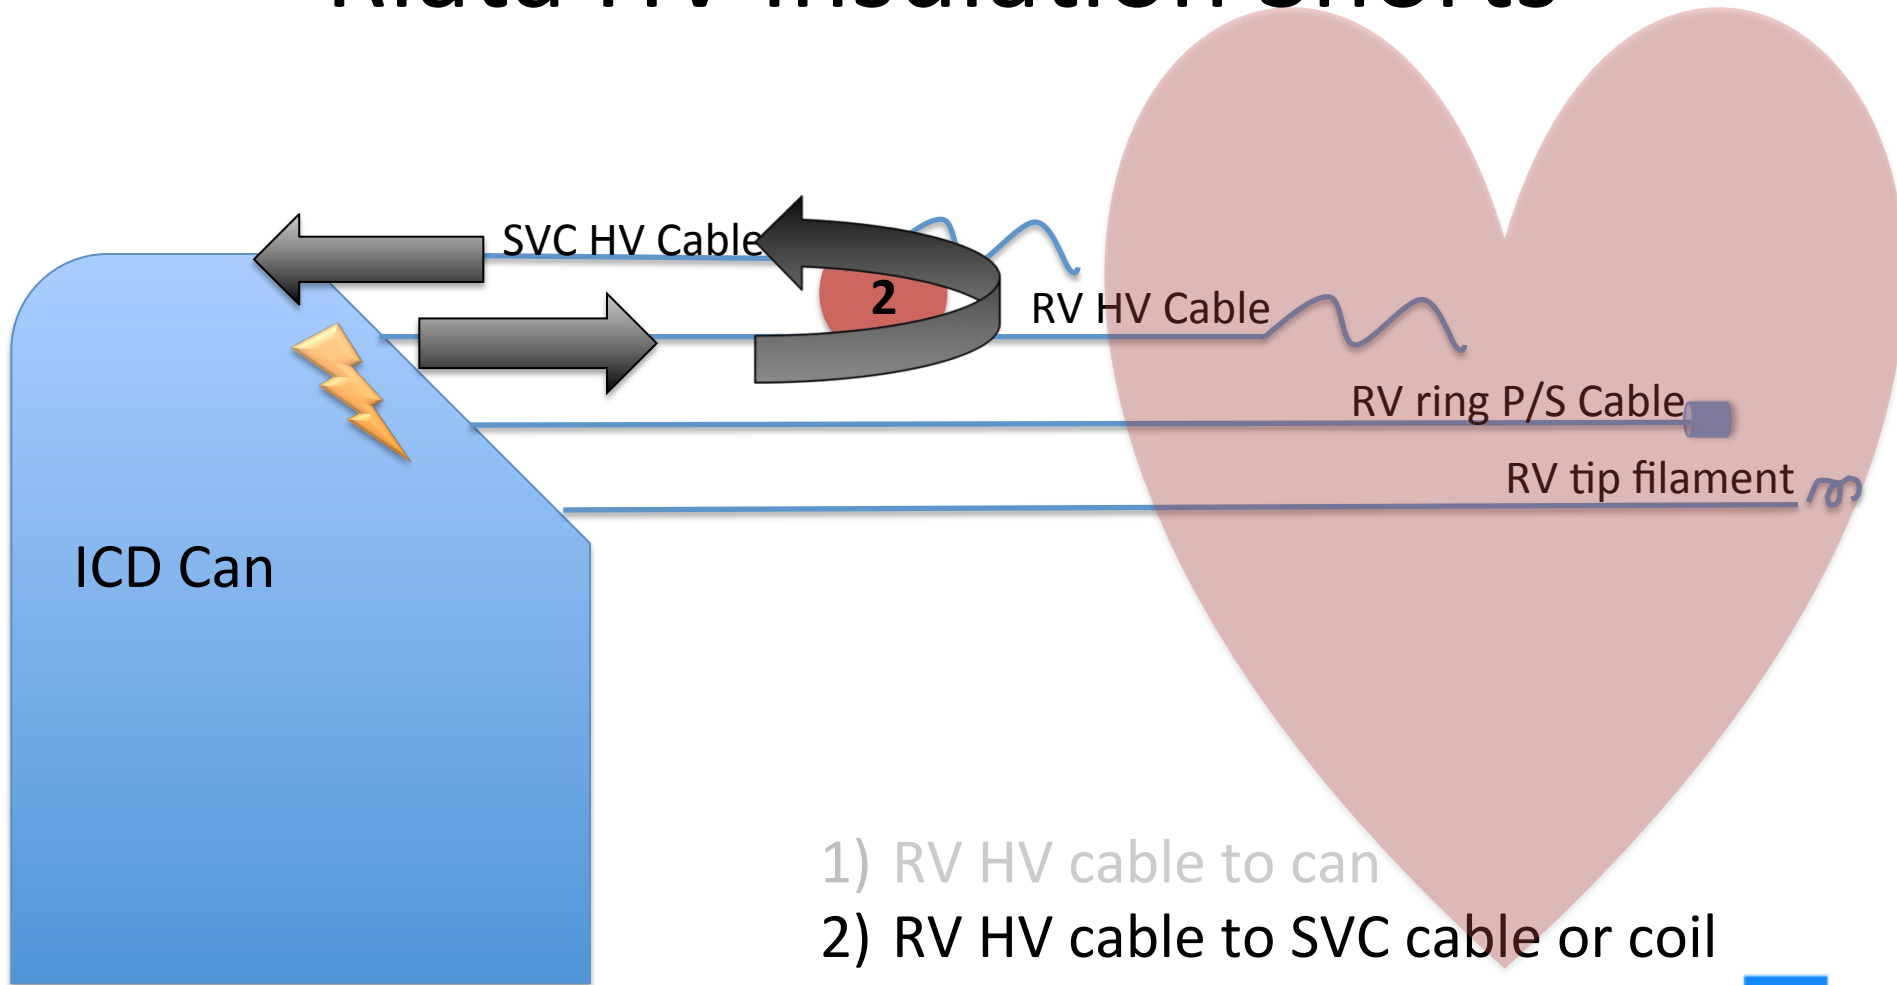

Programming SVC Coil out of system may mitigate failure



Riata HV Insulation Shorts

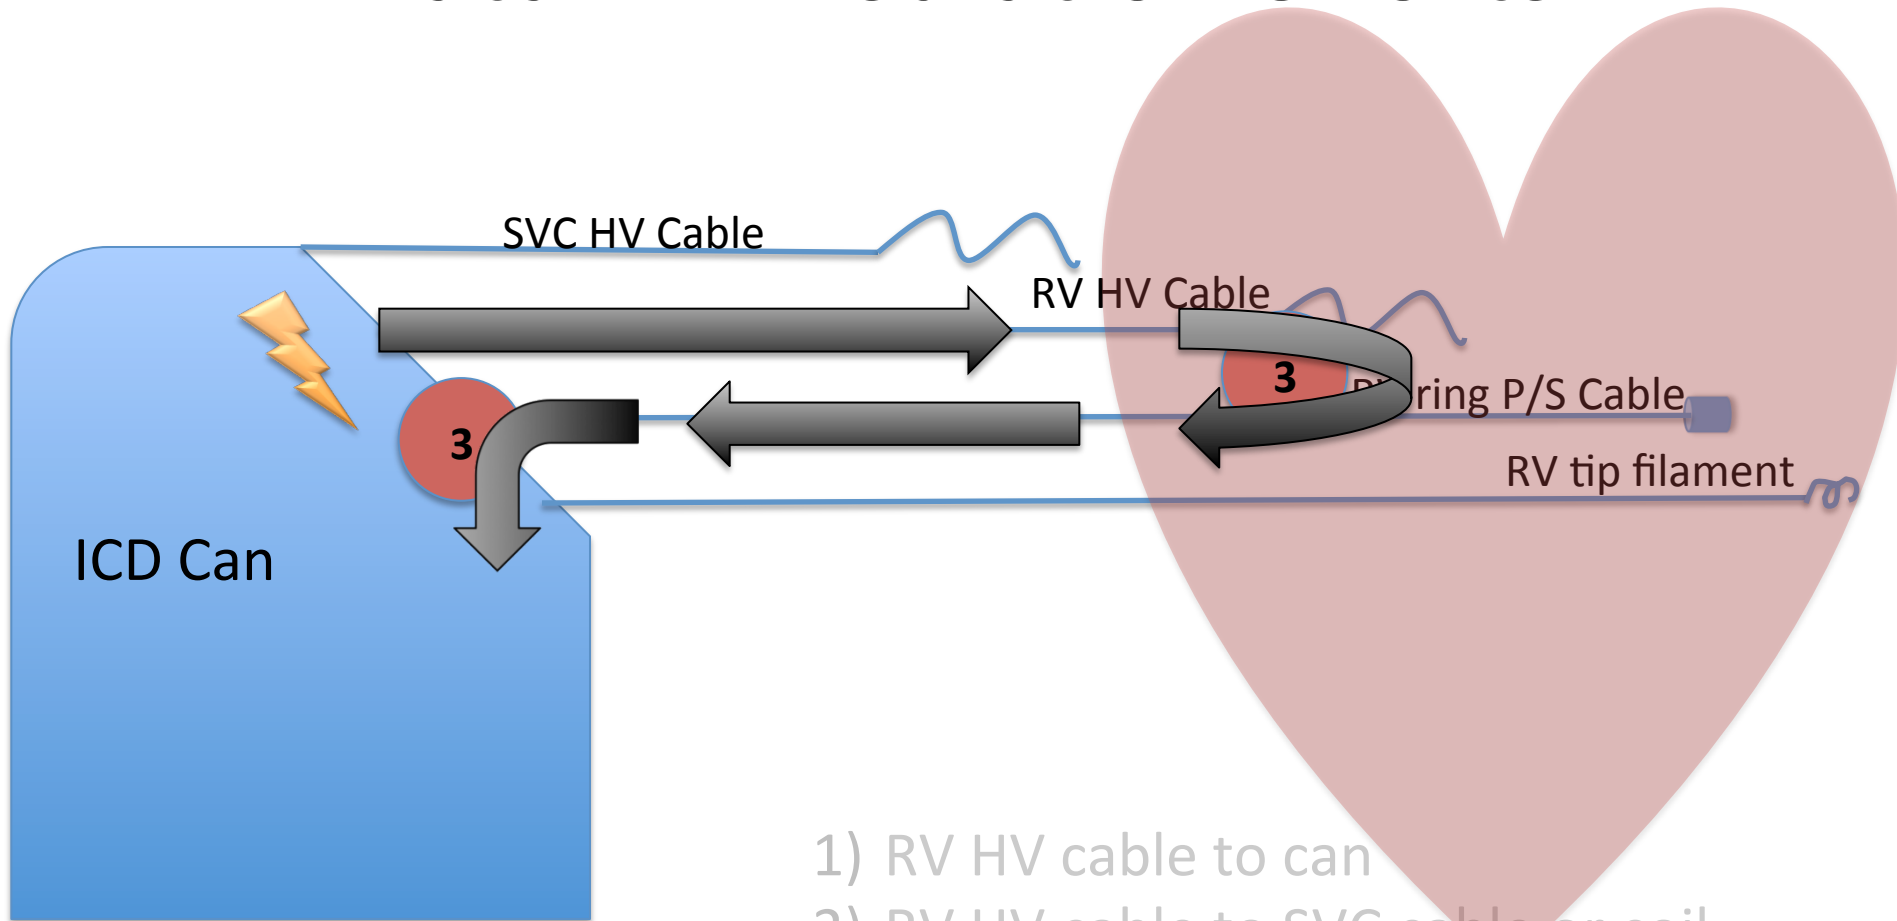

Other variations of #3 exist with alternative return circuit

- 1) RV HV cable to can
- 2) RV HV cable to SVC cable or coil
- 3) RV Ring P/S cable to RV HV cable and RV ring to can

©Edward J. Schloss MD FACC FHRS

